

## Development of an ultrastable laser at 1550 nm

**J De Martin Jr**<sup>1</sup>, **S K N Valappil**<sup>1</sup>, **S T Müller**<sup>1</sup>, **P W Courteille**<sup>2</sup>, **V S Bagnato**<sup>2</sup>,  
**D V Magalhães**<sup>1</sup>

<sup>1</sup> São Carlos School of Engineering /EESC-USP; <sup>2</sup> São Carlos Institute of Physics /IFSC-USP

E-mail: jairdemartinjr@terra.com.br

**Resumo:** Este trabalho aborda o desenvolvimento de um laser de diodo em 1550nm estabilizado contra uma cavidade de alta finesse (pelo menos 250.000). Será relatado os componentes, aparelhos e alguns resultados preliminares para o sistema em construção.

**Palavras-chave:** laser ultra estável, cavidade óptica, estabilização de laser.

**Abstract:** This work deals with the development of a 1550 nm diode laser stabilized against a high finesse cavity (at least 250,000). It reports the components, apparatus and some preliminary results for the system under construction.

**Keywords:** ultra stable laser, optical cavity, laser stabilization.


### 1. INTRODUCTION

Lasers are applied in a wide range of sectors, from industry to high precision physics. To be used in some physics experiments, like high resolution spectroscopy, there is a need for very accurate and stable systems. In this sense is fundamental to reduce the linewidth of the laser system, to be able to resolve certain atomic transitions. Our Reference Systems Group, at USP has been developing such systems with linewidth enough to deal with atomic reference standards [1].

One of the main aspects concerning the quality of a laser is its linewidth. For a free-running laser, this characteristic can be on the order of megahertz. There are several techniques to reduce the linewidth, for example, the use of an extended cavity for a diode laser (ECDL) [2] or servo the laser to a high finesse Fabry-Perot cavity (PDH technique) [3].

The use of external Fabry-Perot cavities to reference laser systems is one of the most common techniques for stabilizing ultra stable lasers [4].

On the other hand, special attention should be devoted when preparing the mechanical structure to isolate the cavity, since the deformations in the cavity degrade the stabilization system [5], and a temperature control in the mK range is crucial, in order to maintain the cavity around the most stable region of operation. Also, the quality of the controllers has a fundamental whole in the laser stabilization, where a reflection from the optical cavity is used to lock on the desired frequency. The aim of this work is to develop a system able to stabilize a diode laser at 1550 nm in a sub-hertz level linewidth. Figure 1 summarizes the system.

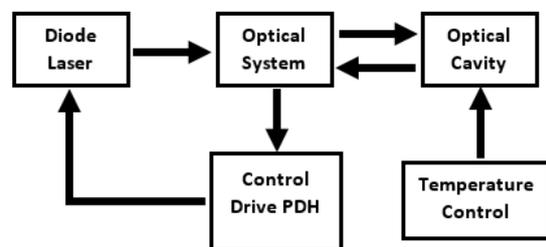

**Figure 1** - General scheme of the parts for the ultra stable laser system at 1550 nm.

## 2. SYSTEM DESCRIPTION

Following are presented the components for the laser stabilization system.

### 2.1. Diode Laser

The system has a diode laser of 1550 nm with linewidth in free-running regime of 1 kHz (RIO Orion Laser). The laser parameter settings (temperature and current) are set through a SPI / USB interface with the computer. In addition the laser has a modulation input used as corrective feedback.

### 2.2. Optical System

In order to stabilize the laser in the sub-hertz level is essential to use an optical cavity (FPC – Fabry-Perot cavity) for reference. The cavity used has a finesse 250,000 and length of 10 cm.


The big issue for the laser stabilization is the injection of laser light into the optical cavity and the optical system should be done to achieve the best possible impedance and mode matching for the cavity.

### 2.3. Vacuum chamber

In order to provide a shielding for temperature stabilization, a vacuum chamber is used to protect the optical cavity. The chamber used is also involved with an acrylic blanket to increase their isolation with the variation of ambient temperature. In addition there are four Peltier elements coupled to the chamber for temperature control.

### 2.4. Mechanical Insulation System

The vacuum chamber, diode laser and the optical system are being mounted on a breadboard attached to a high isolation passive platform (Minus K). This platform performs isolation through a negative constant spring system, which provides excellent isolation down to 0.5 Hz. In addition the entire system is placed in an acoustic box to prevent coupling of noise. Figure 2 illustrates the system being placed.

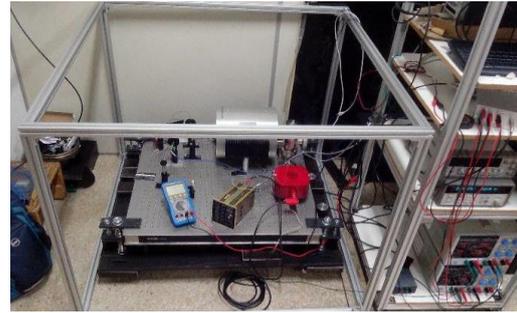


**Figure 2** – Vibration isolation platform surrounded by the cage that supports the plaques for general protection.

It is noteworthy that the platform used has an acceptable weight range of 164 - 239 kg i.e. the optical table over the vacuum chamber is not sufficient to achieve the minimum weight limit, therefore, steel bars were added to the system to work in nominal mass of the platform. This provides a good margin for additional components and, at the same time, keeps the mass center of the system very low.

### 2.5. Laser locking system

To lock the laser, we will use the Pound Drever Hall technique, shown schematically in figure 3.

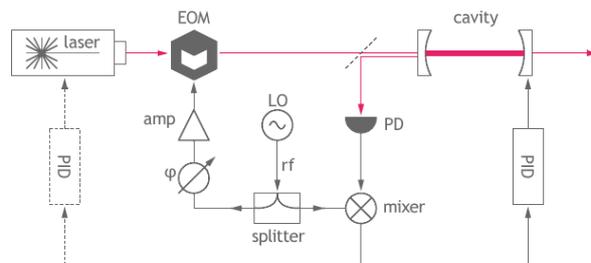


**Figure 3** – Schematic for the Pound Drever Hall technique [6] being mounted to lock the laser to the FPC.

Basically, this technique is achieved through modulation and demodulation of a signal in the megahertz order in the laser light. A radio frequency signal is injected through an electro-optic modulator, which induces sidebands to the laser light. The light of the optical cavity


resonance and the sidebands are collected by a photo-detector and demodulated with a mixer.

### 3. TEMPERATURE CONTROL OF THE VACUUM CHAMBER

To implement the temperature control is essential to know the thermal behavior of the vacuum chamber. So it is necessary to take into account the plant parameters. The technique used is the relay method, which induces a relay-type non-linearity in the plant, to determine the parameters of the descriptive function [7]. The output is basically a sinusoidal signal, with time and amplitude depending on the input signal (relay signal). Figure 4 shows a control loop using this technique and figure 5 illustrates the relay signal and the plant response.

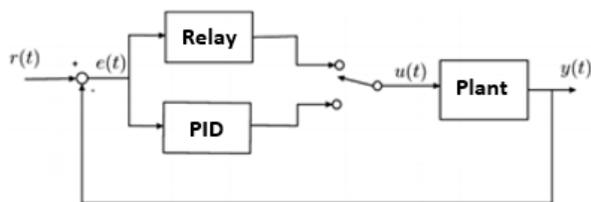

**Figure 4** - Loop Control used to determine the plant characteristics using a relay-type non-linearity.

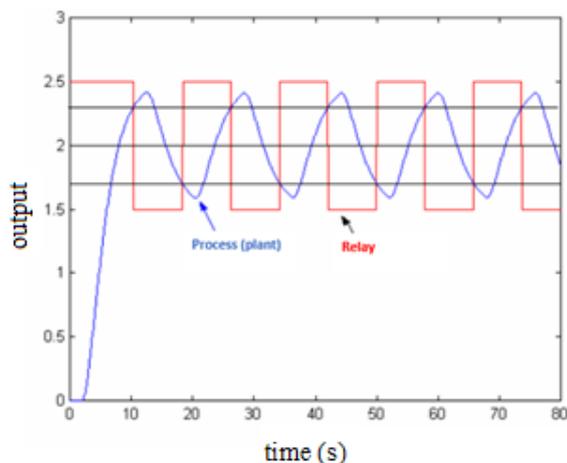


**Figure 5** - Relay signal and plant response.

The initial focus was to understand system behavior as well as their parameters, critical gain and critical period, with these two parameters the

gains Proportional, Integral and Derivative are calculated using the method of Ziegler-Nichols [8].


### 4. CURRENT RESULTS

The optical table assembly has been completed, as shown in figure 6.

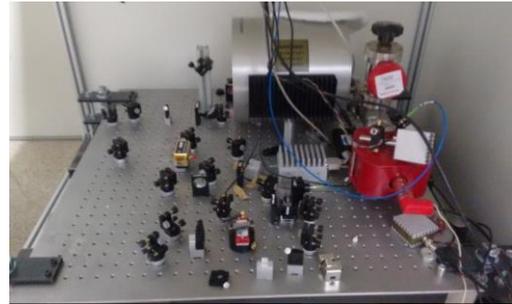


**Figure 6** – Image of the optical bench with the diode laser, FPC and all the optomechanical parts for subsystems.

By adjusting the alignment of the laser beam at the entrance of the cavity and modulating the laser into current, we can visualize the transmission signal of the optical cavity represented in figure 7, with some resonant modes appearing as thin lines over the background noise.

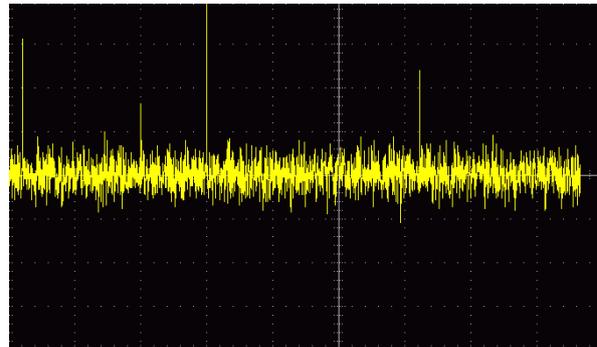

**Figure 7** – Transmission signal of the optical cavity. The thin bigger lines are the resonant modes of the cavity produced with laser frequency modulation.

The temperature control of the vacuum chamber was first implemented using LabView platform with a data acquisition board PCI-6259, figure 8 shows the setup.

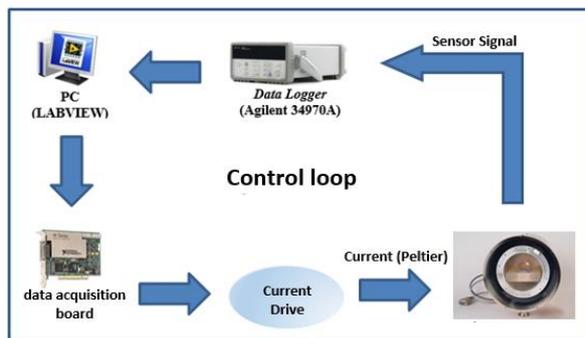

**Figure 8** – Setup of temperature control of vacuum chamber

The temperature variation in the vacuum chamber is detected using a thermistor (sensor) and a data logger (Agilent 34970A). The PID control function is implemented in the computer through LabView software. The output signal from the controller (voltage) is sent to a current driver via analog channel (PCI-6259). The current drives the actuator (Peltier) to heat or cool the vacuum chamber.

By adjusting the PID controller gains the thermal stability found is already under 10 mK variation.

## 5. CONCLUSION

We present the actual status of development for an ultra stabilized laser at 1550nm. The mechanical assembly and temperature control are being finalized. With respect to the cavity transmission signal, the observed noise can degrade the spectral quality of the laser, since the goal is to achieve a line width in the order of mHz. A possible source of noise may be external noise, since the acoustic box is not yet closed. With the reflection signal from the optical cavity it will be possible to close the box and lock the laser, so it is expected to obtain a smaller noise. The next steps concerns the design of the loop filter, characterize the acoustic and mechanical vibration insulation system and the ultra stable laser.

## 6. REFERENCES

- [1] De Martin Jr J, Pechoneri R D, Otoboni F A, Müller S T, Bagnato V S and Magalhães D V 2012 Development of a Mobile Atomic Frequency Standard based on Cold Atoms *Latin America Optics and Photonics Conference*, paper **LM2A.4**.
- [2] Fleming M and Mooradian A 1981 Spectral characteristics of external-cavity controlled semiconductor lasers in Quantum Electronics *IEEE Journal of Quantum Electronics* **17** 44-59.
- [3] Black E. D 2001 An introduction to Pound–Drever–Hall laser frequency stabilization *American Journal of Physics* **69** 79-87.
- [4] Saleh B E A and Teich M C 1991 Fundamentals of Photonics *John Wiley & Sons* **1** 947.
- [5] Millo J, Magalhães D V, Mandache C, Le Coq Y, English E M L, Westergaard P G, Lodewyck J, Bize S, Lemonde P and Santarelli G 2009 Ultrastable lasers based on vibration insensitive cavities *Physical Review A* **3** 8.
- [6] Image available in: <http://www.qubig.com/pound-drever-hall.htm>.
- [7] Almeida M A and Prado M L M 2011 Identificação de uma planta térmica através do método do relé *Sbmac* 351-354.
- [8] Ziegler J B and Nichols N B 1942 Optimum settings for automatic controllers *ASME Transactions* **64** 759-768.